

Application note No. 3034

NucleoCounter® NC-3000™

Viability and Cell Count - Method 2 Assay with Via1-Cassette™

Product description

The NucleoCounter® NC-3000™ system enables the user to perform automated cell counting and analyses of a broad range of mammalian cells.

Application

Method 2 Assay is an alternative analysis to address changes triggered by prolonged cell incubation in bioreactors. The Via1-Cassette™ used together with the NucleoCounter® NC-3000™ facilitates determination of viability and concentration of cell suspensions by measuring cell counts (total and non-viable) per volume in one simple step.

Introduction

Cells cultivated in bioreactors for long periods (e.g. <240h) without media exchange will tend to show unusual

fluorescence patterns of Acridine Orange (AO) and DAPI when compared to fresh samples. This includes formation of small cell-like objects positive for AO but negative for DAPI. The opposite can also be true, with events that are positive for DAPI or Hoechst but negative for AO.

Method 2 accounts for presence of small cell-like objects by allowing inclusion of dim fluorescence intensities that would otherwise be excluded as debris. Also, it permits inclusion of cells stained only with DAPI but not with AO. Note that Method 2 is a more permissive analysis and should only be used in cases where small cell-like objects positive for AO or DAPI are expected.

ProcedureMaterials needed

- Cell sample to be counted
- Via1-Cassette™

1. Engage NucleoView and select the “**Viability and Cell Count – Method 2 Assay**” and sample unit **Via1-Cassette™**. If applicable, insert Sample ID.
2. Mix the cell suspension by inversion or flicking in order to obtain a homogenous suspension.
3. Load a **Via1-Cassette™** by inserting its tip into the cell suspension and pressing the piston.
4. Immediately place the loaded **Via1-Cassette™** in the **NucleoCounter® NC-3000™**, and press RUN.

After approximately 1 minute the viability (in percent) and the concentrations (cells/mL) of all cells are displayed in the result fields. If the cell sample has been further diluted or concentrated and the user has entered the volumes into the user interface, the returned cell concentration will be for the original cell concentration.

Notes

To assure reliable results, the cell concentration of the counted cell suspension should be in the range of 5·10⁴ cells/ml to 5·10⁶ cells/ml. If the cell concentration is above 5·10⁶ cells/ml, the cell suspension can be diluted with growth media or PBS to achieve the desired concentration. If the concentration of cells is below 5·10⁴ cells/ml, it may be increased by centrifugation followed by resuspension of the pellet using growth media or PBS.

Method 2 does not distinguish between small cell-like objects and enucleate AO-positive cellular debris. If cellular debris is present in the sample and the aim is to include only nucleated events, we recommend switching to the “**Aggregated Cell Assay**”. In such case, note that nuclei-based cell count in samples containing vesicular debris might differ from results generated using a light microscopy-based method, which tend to count enucleate events as cells

Viability

The viability is calculated by the NucleoView NC-3000™ software as follows:

$$\% \text{ viability} = \frac{C_t - C_{nv}}{C_t} \cdot 100\%$$

% viability


The percentage of viable cells in the cell suspension

C_t

The total concentration of cells

C_{nv}

The concentration of non-viable cells

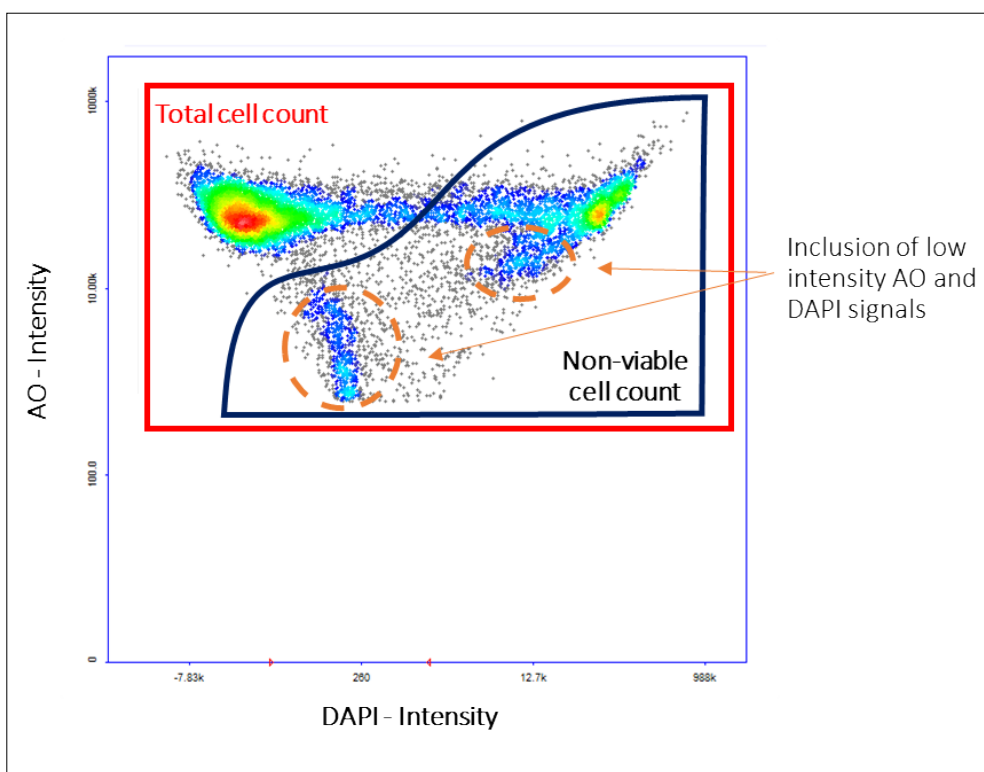

Method 2 analysis includes low intensity Acridine Orange (AO) and DAPI. Cells were harvested, loaded into a Via1-Cassette™ and analyzed using the Viability and Cell Count – Method 2 Assay. Total cell count includes all identified objects, regardless of intensity differences (left). Dead cell count includes low intensity AO together with low and high intensity DAPI.

Troubleshooting

Inaccurate and imprecise counting:

When setting up a new cell line it is important to inspect that the cell line is counted correctly. The cells included in the total count can be marked by clicking on the overlay button in the bottom right corner of the image. Visual inspect the image to evaluate in the vast majority of the cells has been counted correctly. If this is not the case right click on the image file in question and choose "Show Raw Data". Inspect the gates displayed in the Plot Manager. If the gating is inappropriate right click on the image file in question again and choose "Start Protocol Adaptation Wizard". Adapt the gate(s) to cover the cell population (do not include debris and very large objects) and save the changes to a new protocol. Note that the user is responsible for defining appropriate gating of the particular cell line.

Handling and storage

For handling and storage of ChemoMetec instruments and reagents, cassettes and NC-Slides refer to the corresponding product documentation. For other reagents refer to the material data sheet from the manufacturer of the reagents and chemicals.

Warnings and precautions

For safe handling and disposal of the ChemoMetec reagents, cassettes and NC-slides refer to the corresponding product documentation and the NucleoCounter® NC-3000™ user's guide. For other reagents refer to the safety data sheet from the manufacturer of the reagents and chemicals required for this protocol. Wear suitable eye protection and protective clothes and gloves when handling biologically active materials.

Limitations

The NucleoCounter® NC-3000™ system is FOR RESEARCH USE ONLY. NOT FOR DIAGNOSTIC OR THERAPEUTIC USE. The results presented by the NucleoCounter® NC-3000™ system depend on correct use of the reagents, NC-slide and the NucleoCounter® NC-3000™ instrument and might depend on the type of cells being analyzed. Refer to the NucleoCounter® NC-3000™ user's guide for instructions and limitations.

Liability disclaimer

This application note is for RESEARCH PURPOSES ONLY. It is not intended for food, drug, household, or cosmetic use. Its use must be supervised by a technically qualified individual experienced in handling potentially hazardous chemicals. The above information is correct to the best of our knowledge. Users should make independent decisions regarding completeness of the information based on all sources available. ChemoMetec A/S shall not be held liable for any damage resulting from handling or contact with the above product.

Product disclaimer

ChemoMetec A/S reserves the right to introduce changes in the product to incorporate new technology. This application note is subject to change without notice.

Copyright

Copyright © ChemoMetec A/S 2003. All rights reserved. No part of this publication may be reproduced, stored in a retrieval system, or transmitted in any form or by any means, electronic, mechanical, photocopying, recording or otherwise, without the prior written consent of ChemoMetec A/S, Gydevang 43, DK-3450 Allerød, Denmark.